

Main Body Bifurcate Stent-Graft

Leg Extension Stent-Graft

Aortic Outer Diameter (Proximal Neck Angle ≤ 60°)	Proximal Landing Zone Minimum Length	Proximal Diameter	Contralateral Length	Profile	Catalog Reference
17-18	15	20	80	18 Fr	28-B2-20-080U
	15	20	100	18 Fr	28-B2-20-100U
	15	20	120	18 Fr	28-B2-20-120U
18-19	15	22	80	18 Fr	28-B2-22-080U
	15	22	100	18 Fr	28-B2-22-100U
	15	22	120	18 Fr	28-B2-22-120U
19-21	15	24	80	18 Fr	28-B2-24-080U
	15	24	100	18 Fr	28-B2-24-100U
	15	24	120	18 Fr	28-B2-24-120U
21-23	15	26	80	18 Fr	28-B2-26-080U
	15	26	100	18 Fr	28-B2-26-100U
	15	26	120	18 Fr	28-B2-26-120U
23-25	15	28	80	18 Fr	28-B2-28-080U
	15	28	100	18 Fr	28-B2-28-100U
	15	28	120	18 Fr	28-B2-28-120U
25-27	15	30	80	19 Fr	28-B2-30-080U
	15	30	100	19 Fr	28-B2-30-100U
	15	30	120	19 Fr	28-B2-30-120U
27-30	15	33	80	19 Fr	28-B2-33-080U
	15	33	100	19 Fr	28-B2-33-100U
	15	33	120	19 Fr	28-B2-33-120U
30-32	15	36	80	19 Fr	28-B2-36-080U
	15	36	100	19 Fr	28-B2-36-100U
	15	36	120	19 Fr	28-B2-36-120U

Iliac Inner Diameter	Iliac Landing Zone Minimum Length	Leg Extension Distal Diameter	Covered Length	Profile	Catalog Reference
8	10	9	80	13 Fr	28-L2-09-080U
	10	9	100	13 Fr	28-L2-09-100U
	10	9	120	13 Fr	28-L2-09-120U
	10	9	140	13 Fr	28-L2-09-140U
	10	9	160	13 Fr	28-L2-09-160U
	10	11	80	13 Fr	28-L2-11-080U
9	10	11	100	13 Fr	28-L2-11-100U
	10	11	120	13 Fr	28-L2-11-120U
	10	11	140	13 Fr	28-L2-11-140U
	10	11	160	13 Fr	28-L2-11-160U
	10	13	80	13 Fr	28-L2-13-080U
	10	13	100	13 Fr	28-L2-13-100U
10-11	10	13	120	13 Fr	28-L2-13-120U
	10	13	140	13 Fr	28-L2-13-140U
	10	13	160	13 Fr	28-L2-13-160U
	10	15	80	13 Fr	28-L2-15-080U
	10	15	100	13 Fr	28-L2-15-100U
	10	15	120	13 Fr	28-L2-15-120U
12-13	10	15	140	13 Fr	28-L2-15-140U
	10	15	160	13 Fr	28-L2-15-160U
	15	17	80	14 Fr	28-L2-17-080U
	15	17	100	14 Fr	28-L2-17-100U
	15	17	120	14 Fr	28-L2-17-120U
	15	17	140	14 Fr	28-L2-17-140U
14-15	15	17	160	14 Fr	28-L2-17-160U
	15	20	80	14 Fr	28-L2-20-080U
	15	20	100	14 Fr	28-L2-20-100U
	15	20	120	14 Fr	28-L2-20-120U
	15	20	140	14 Fr	28-L2-20-140U
	15	20	160	14 Fr	28-L2-20-160U
16-17	15	24	80	14 Fr	28-L2-24-080U
	15	24	100	14 Fr	28-L2-24-100U
	15	24	120	14 Fr	28-L2-24-120U
	15	24	140	14 Fr	28-L2-24-140U
	15	24	160	14 Fr	28-L2-24-160U
	18-20	15	24	80	14 Fr
15		24	100	14 Fr	28-L2-24-100U
15		24	120	14 Fr	28-L2-24-120U
15		24	140	14 Fr	28-L2-24-140U
15		24	160	14 Fr	28-L2-24-160U

Straight Extension Stent-Graft\*


Iliac Inner Diameter	Iliac Landing Zone Minimum Length	Proximal and Distal Diameter	Covered Length	Profile	Catalog Reference
8	10	9	80	13 Fr	28-S2-09-080U
9	10	11	80	13 Fr	28-S2-11-080U
10-11	10	13	80	13 Fr	28-S2-13-080U

\* Straight Extension Stent-Grafts indicated for use only with previously implanted Leg Extension Stent-Grafts with the same distal diameter.

## Proximal Cuff Extension Stent-Graft

Aortic Outer Diameter (Proximal Neck Angle ≤ 60°)	Proximal Landing Zone Minimum Length	Proximal and Distal Diameter	Covered Length	Profile	Catalog Number
17-18	15	20	40	18 Fr	28-C2-20-040U
	15	20	55	18 Fr	28-C2-20-055U
	15	20	70	18 Fr	28-C2-20-070U
18-19	15	22	40	18 Fr	28-C2-22-040U
	15	22	55	18 Fr	28-C2-22-055U
	15	22	70	18 Fr	28-C2-22-070U
19-21	15	24	40	18 Fr	28-C2-24-040U
	15	24	55	18 Fr	28-C2-24-055U
	15	24	70	18 Fr	28-C2-24-070U
21-23	15	26	40	18 Fr	28-C2-26-040U
	15	26	55	18 Fr	28-C2-26-055U
	15	26	70	18 Fr	28-C2-26-070U
23-25	15	28	40	18 Fr	28-C2-28-040U
	15	28	55	18 Fr	28-C2-28-055U
	15	28	70	18 Fr	28-C2-28-070U
25-27	15	30	40	19 Fr	28-C2-30-040U
	15	30	55	19 Fr	28-C2-30-055U
	15	30	70	19 Fr	28-C2-30-070U
27-30	15	33	40	19 Fr	28-C2-33-040U
	15	33	55	19 Fr	28-C2-33-055U
	15	33	70	19 Fr	28-C2-33-070U
30-32	15	36	40	19 Fr	28-C2-36-040U
	15	36	55	19 Fr	28-C2-36-055U
	15	36	70	19 Fr	28-C2-36-070U

## Catalog Reference Key

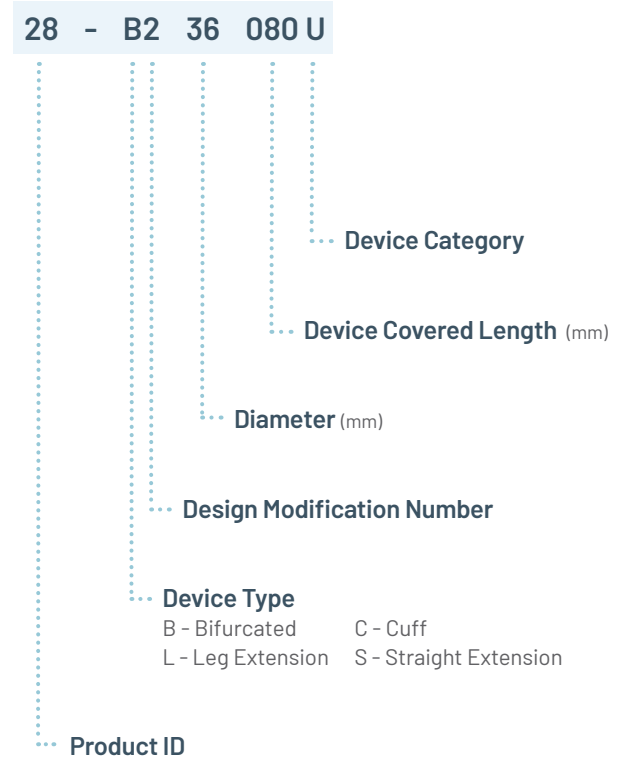

All measurements in mm unless otherwise specified.

## Indications for Use

The **TREO® ABDOMINAL STENT-GRAFT SYSTEM** is indicated for use in the endovascular treatment of patients with infrarenal abdominal aortic and aorto-iliac aneurysms with the following characteristics:

- ▶ Adequate iliac or femoral access compatible with the required delivery systems and accessories
- ▶ Proximal aortic landing zone with:
  - ▶ Infrarenal landing neck length of ≥ 15mm
  - ▶ Aortic neck diameters ≥ 17mm and ≤ 32mm
  - ▶ Suprarenal neck angle of ≤ 45 degrees
  - ▶ Infrarenal neck angle of ≤ 60 degrees
- ▶ Distal iliac landing zone with:
  - ▶ an inside diameter of 8mm – 13mm and a length of ≥ 10mm or
  - ▶ an inside diameter of > 13mm – 20mm and a length of ≥ 15mm
- ▶ Minimum overall AAA treatment length (proximal landing location to distal landing location) of 13cm
- ▶ Minimum overall length from the lowest renal artery to the aortic bifurcation of 9cm

## terumo-aortic.com

Discover solutions for every segment of the aorta

Please visit our website to learn more information on use, indications, contraindications, warnings/precautions and availability within your market.

Rx Only. Caution: Federal (USA) law restricts this device to sale by or on the order of a physician.

Manufactured by: Bolton Medical Inc, 799 International Parkway, Sunrise, Florida 33325, United States